


[See all 39 Products in Family](#)

TECHSPEC®

304.8mm Dia. λ /20 Fused Silica Optical Flat

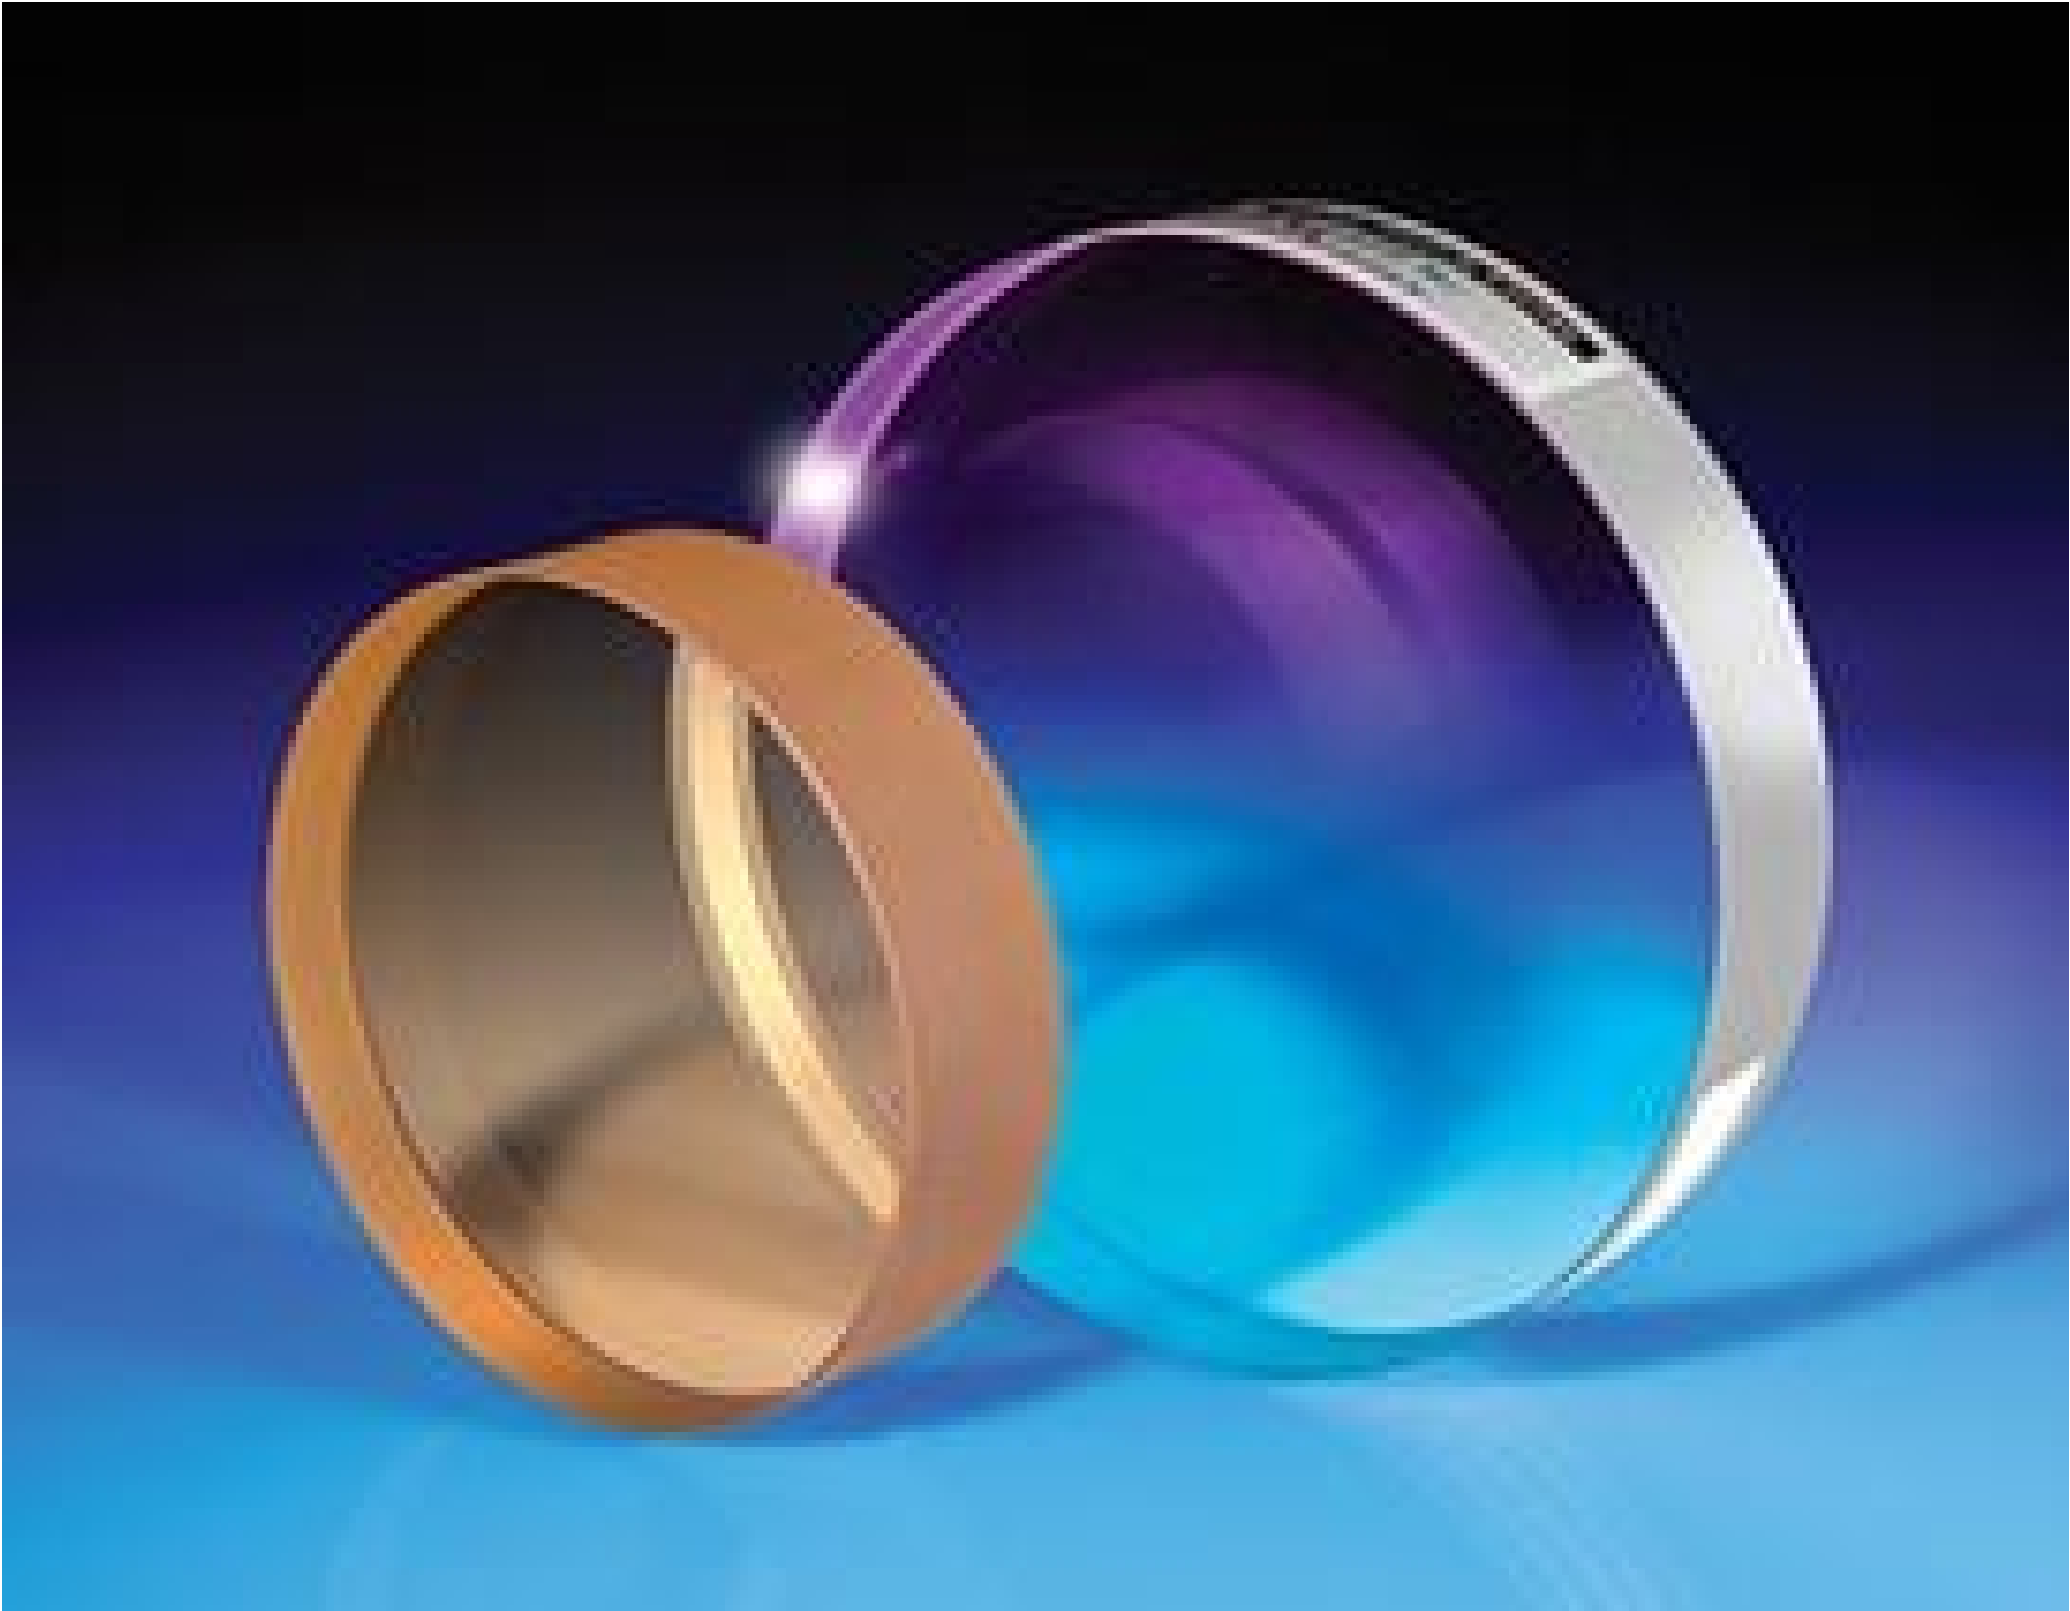

Stock

#65-880-000

10 In Stock

-

1

+

£10,464⁰⁰

ADD TO CART

Volume Pricing	
Qty 1-2	£10,464.00 each
Qty 3-5	£9,296.00 each
Qty 6-9	£8,752.00 each
Need More?	Request Quote

i Prices shown are exclusive of VAT/local taxes

Product Downloads

General	
Interferometry Window	Type:
Includes a certificate of calibration.	Note:

Physical & Mechanical Properties	
274.30	Clear Aperture CA (mm):
12.00 +0.00/-0.04	Diameter (inches):
304.80 +0.00/-1.00	Diameter (mm):
1.50 ±0.10	Thickness (inches):
38.10 ±2.5	Thickness (mm):
≤3	Parallelism (arcmin):
Protective as needed	Bevel:
Single Surface	Construction:
Fine Ground	Edges:
0.16	Poisson's Ratio:
73	Young's Modulus (GPa):
522.00	Knoop Hardness (kg/mm²):

Optical Properties	
Uncoated	Coating:
Clear	Color:
Fused Silica	Substrate: ☐
1.458	Index of Refraction (n _d):
60-40	Surface Quality:
67.8	Abbe Number (v _d):
200 - 2200	Wavelength Range (nm):
λ/20	Surface Flatness (P-V):

Material Properties	
2.20	Density (g/cm³):
0.52 (+5 to +35°C) 0.57 (0 to +200°C) 0.48 (-100 to +200°C)	Coefficient of Thermal Expansion CTE (10 ⁻⁶ /°C):

Regulatory Compliance	
Compliant	RoHS 2015:
Compliant	Reach 211:
View	Certificate of Conformance:

Product Details

- Sizes Ranging from ½" Diameter to 14" Diameter
- Each λ/20 Flat 76.2mm and Larger Includes a Certificate of Calibration
- Available with Standard Metallic Mirror Coatings: [λ/10](#) and [λ/20 Mirrors](#)

TECHSPEC® Single Surface Optical Flats are used as a reference (test plate) against which the flatness of an unknown surface may be compared. Each piece is precision polished by our master opticians and tested on a Zygo interferometer to insure the surface flatness. The secondary surfaces of our single surface flats are pitch polished to window quality for viewing the interference pattern. TECHSPEC Single Surface Optical Flats ship in a durable storage case for permanent protection. λ/20 flats that are 76.2mm or larger also include a certificate of calibration.